

# **NZVP Quality Assurance Programme**




## **Example Report**

### **Chemistry**






### Albumin (g/L)

<b>Your result</b>	29	
<b>Mean of all results</b>	30	<b>Results excluded: 2</b>
- Standard deviation	1.71	
- %CV	5.77	
<b>Mean of Your analyser results</b>	29	<b>Results excluded: 0</b>
- Standard deviation	1.44	
- %CV	4.89	
<b>Your standard deviation index</b>	0.00	
<b>NZVP result</b>	35.6	

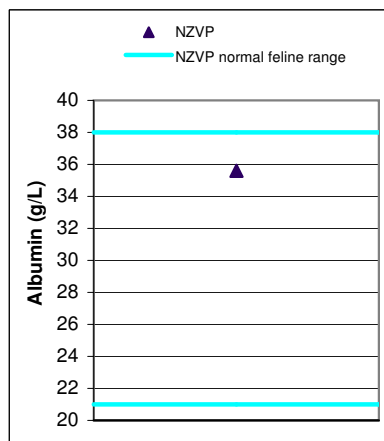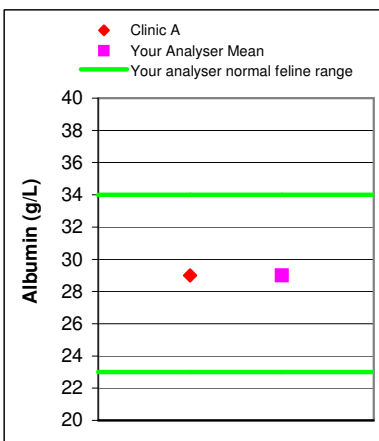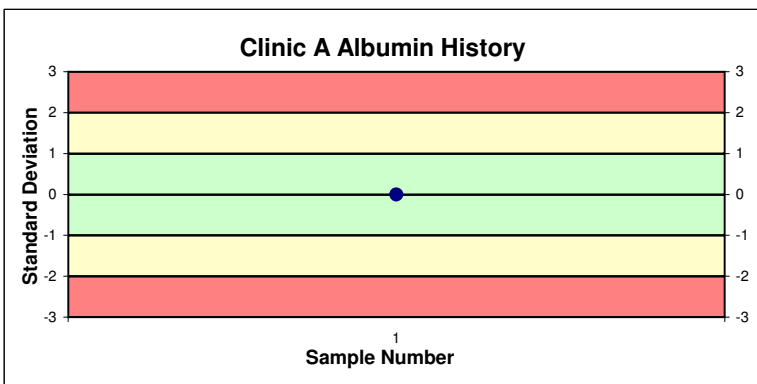

### ALP (U/L)

<b>Your result</b>	33	
<b>Mean of all results</b>	54	<b>Results excluded: 4</b>
- Standard deviation	3.59	
- %CV	6.67	
<b>Mean of Your analyser results</b>	54	<b>Results excluded: 4</b>
- Standard deviation	3.71	
- %CV	6.84	
<b>Your standard deviation index</b>	-5.66	
<b>NZVP result</b>	43	

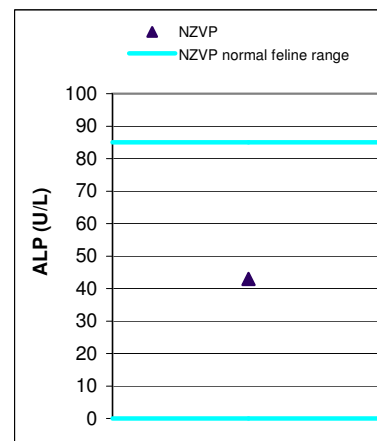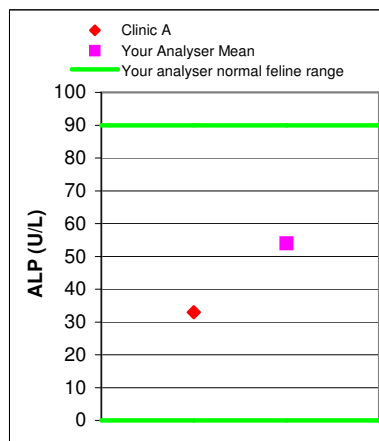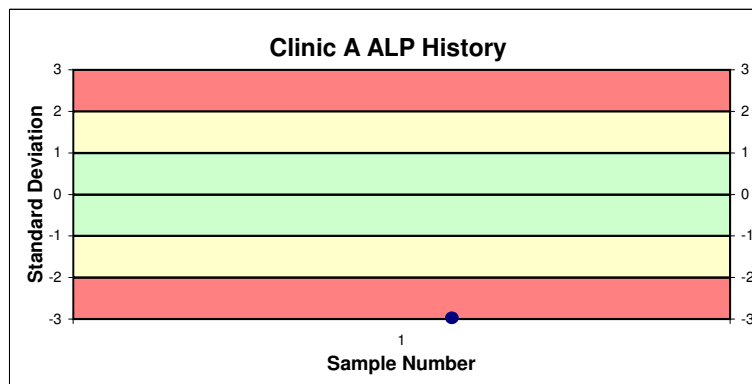







Your result has been excluded from statistics calculations

### ALT (U/L)

<b>Your result</b>	70	
<b>Mean of all results</b>	69	<b>Results excluded: 0</b>
- Standard deviation	3.65	
- %CV	5.27	
<b>Mean of Your analyser results</b>	69	<b>Results excluded: 0</b>
- Standard deviation	3.09	
- %CV	4.49	
<b>Your standard deviation index</b>	0.32	
<b>NZVP result</b>	98	

### Amylase (U/L)

<b>Your result</b>	653	
<b>Mean of all results</b>	892	<b>Results excluded: 0</b>
- Standard deviation	143.60	
- %CV	16.10	
<b>Mean of Your analyser results</b>	834	<b>Results excluded: 0</b>
- Standard deviation	128.91	
- %CV	15.46	
<b>Your standard deviation index</b>	-1.40	
<b>NZVP result</b>	1179	

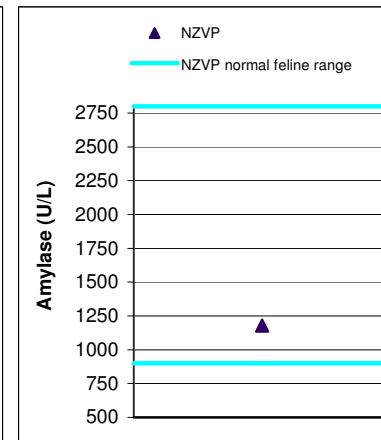
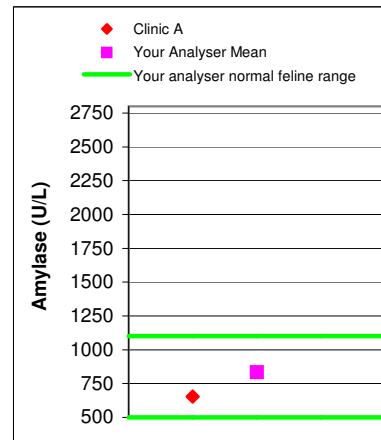
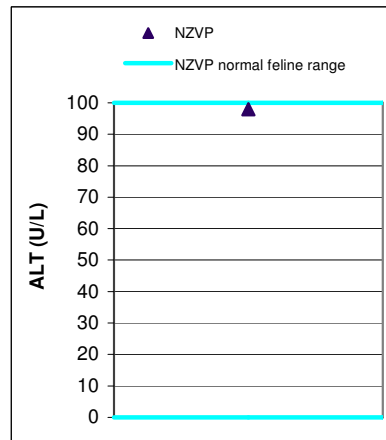
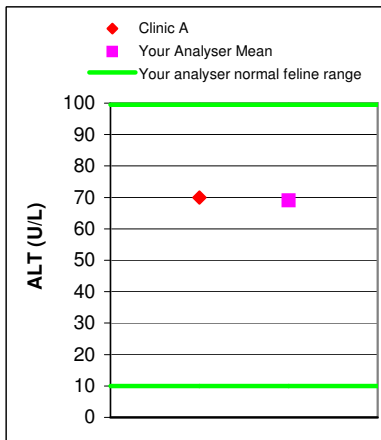
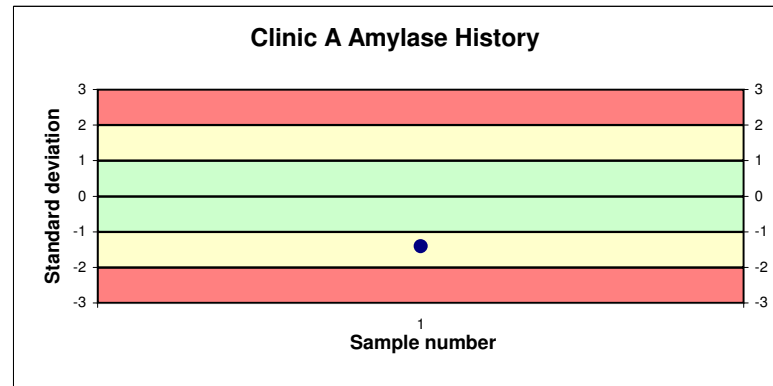
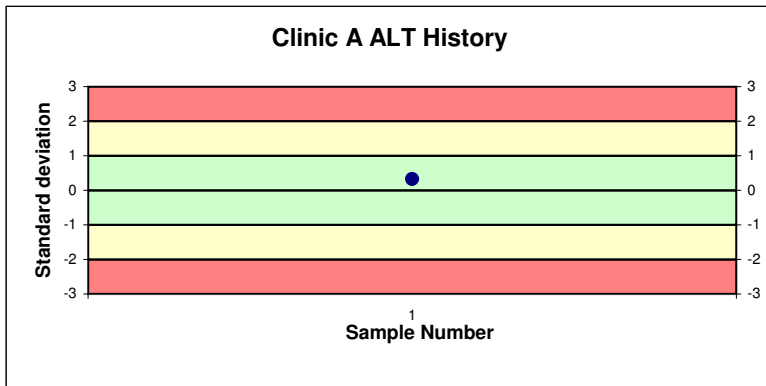


### Bilirubin (umol/L)

<b>Your result</b>	6	
<b>Mean of all results</b>	6.4	<b>Results excluded: 1</b>
- Standard deviation	2.29	
- %CV	36.02	
<b>Mean of Your analyser results</b>	5.5	<b>Results excluded: 1</b>
- Standard deviation	1.20	
- %CV	21.73	
<b>Your standard deviation index</b>	0.42	
<b>NZVP result</b>	1.0	

### Calcium (mmol/L)

<b>Your result</b>	3.10	
<b>Mean of all results</b>	2.82	<b>Results excluded: 1</b>
- Standard deviation	0.20	
- %CV	6.95	
<b>Mean of Your analyser results</b>	2.88	<b>Results excluded: 0</b>
- Standard deviation	0.15	
- %CV	5.14	
<b>Your standard deviation index</b>	1.47	
<b>NZVP result</b>	2.45	

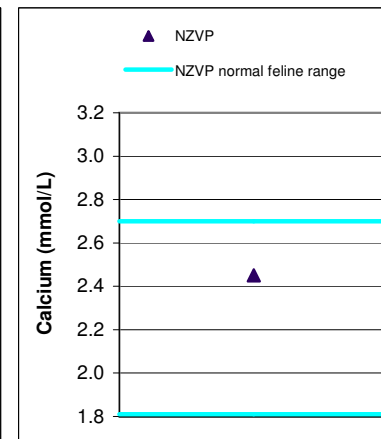
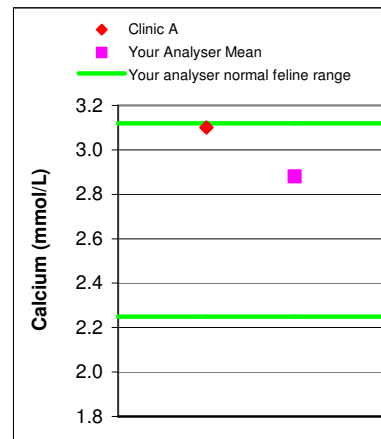
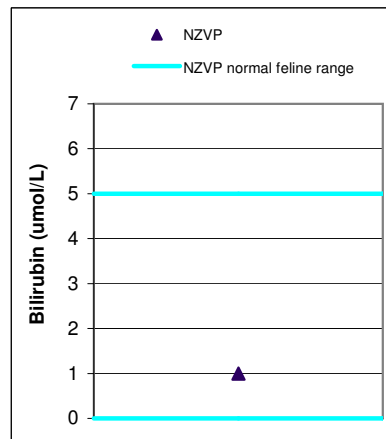
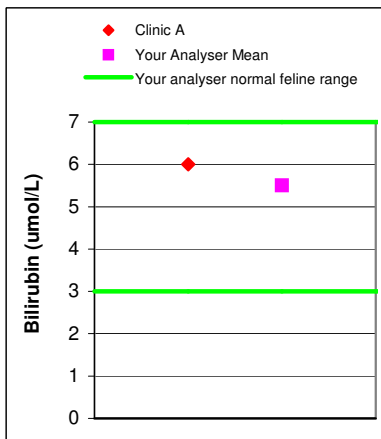
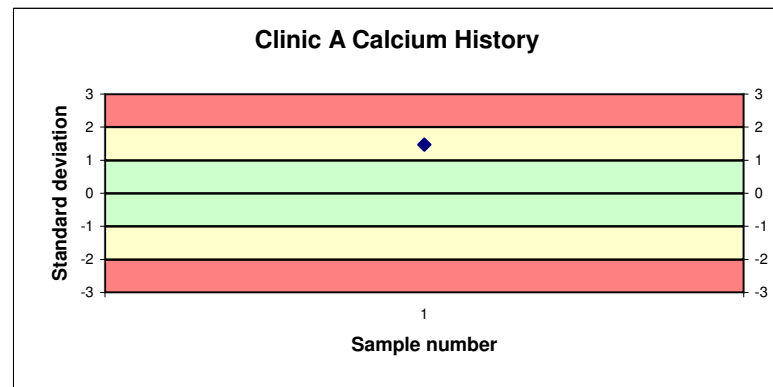
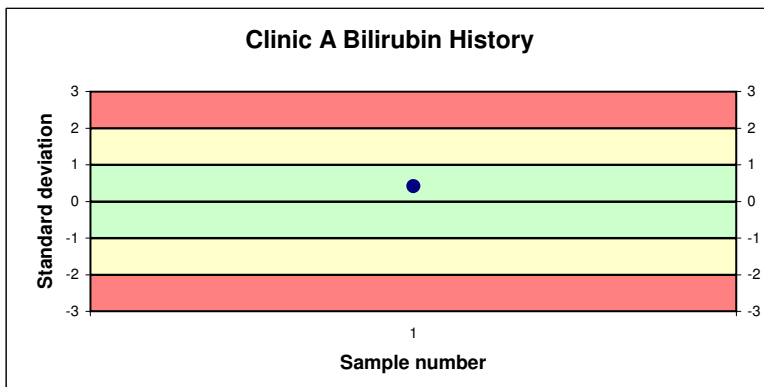


### Cholesterol (mmol/L)

<b>Your result</b>	4.71	
<b>Mean of all results</b>	4.57	<b>Results excluded: 0</b>
- Standard deviation	0.27	
- %CV	5.97	
<b>Mean of Your analyser results</b>	4.70	<b>Results excluded: 0</b>
- Standard deviation	0.24	
- %CV	5.11	
<b>Your standard deviation index</b>	0.04	
<b>NZVP result</b>	4.42	

### Creatinine (umol/L)

<b>Your result</b>	222	
<b>Mean of all results</b>	213	<b>Results excluded: 2</b>
- Standard deviation	11.68	
- %CV	5.50	
<b>Mean of Your analyser results</b>	214	<b>Results excluded: 2</b>
- Standard deviation	11.60	
- %CV	5.41	
<b>Your standard deviation index</b>	0.69	
<b>NZVP result</b>	193	

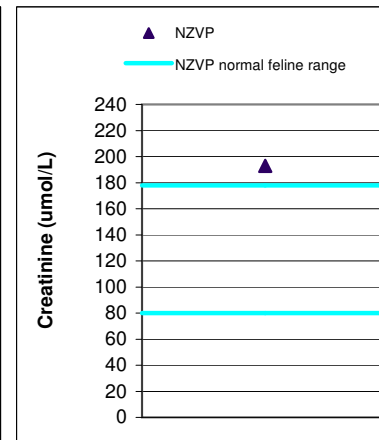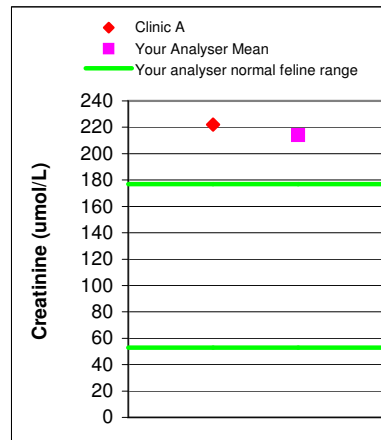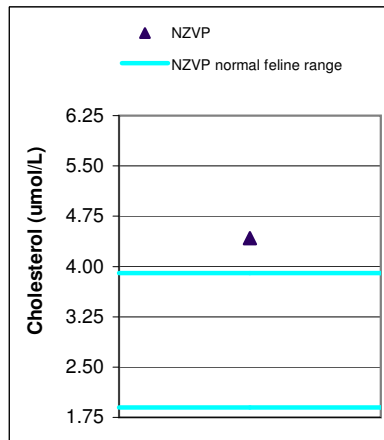
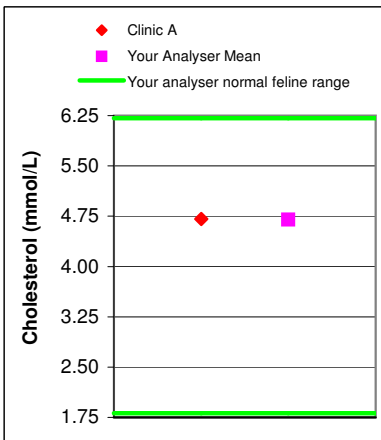
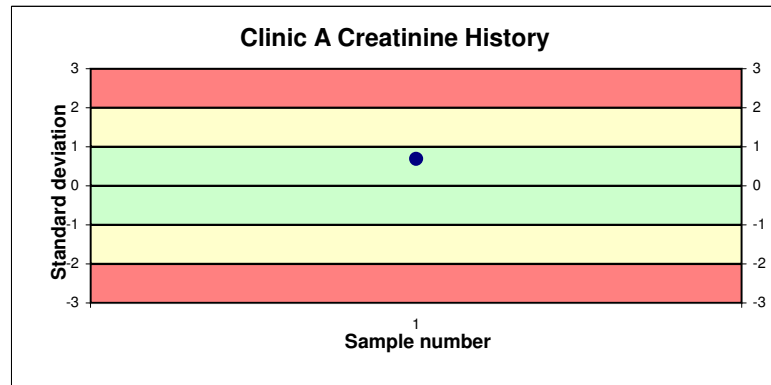
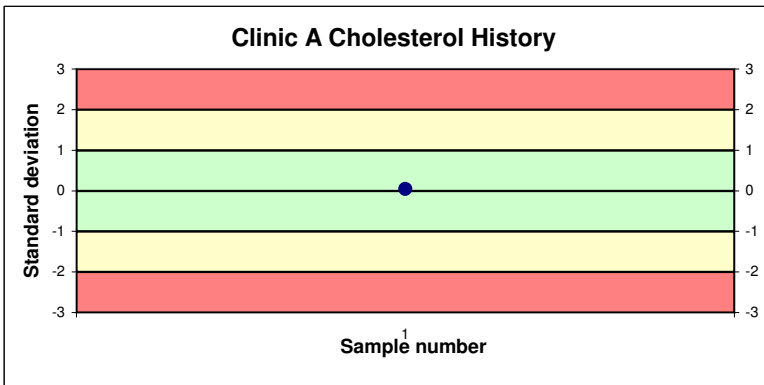


### Glucose (mmol/L)

<b>Your result</b>	4.62	
<b>Mean of all results</b>	4.72	<b>Results excluded: 0</b>
- Standard deviation	0.18	
- %CV	3.87	
<b>Mean of Your analyser results</b>	4.69	<b>Results excluded: 0</b>
- Standard deviation	0.19	
- %CV	4.12	
<b>Your standard deviation index</b>	-0.37	
<b>NZVP result</b>	4.9	

### Phosphate (mmol/L)

<b>Your result</b>	2.65	
<b>Mean of all results</b>	2.68	<b>Results excluded: 2</b>
- Standard deviation	0.06	
- %CV	2.29	
<b>Mean of Your analyser results</b>	2.66	<b>Results excluded: 2</b>
- Standard deviation	0.07	
- %CV	2.58	
<b>Your standard deviation index</b>	-0.14	
<b>NZVP result</b>	2.59	

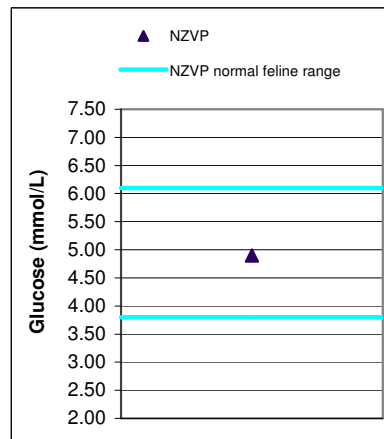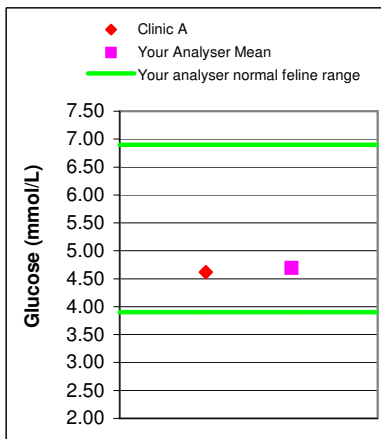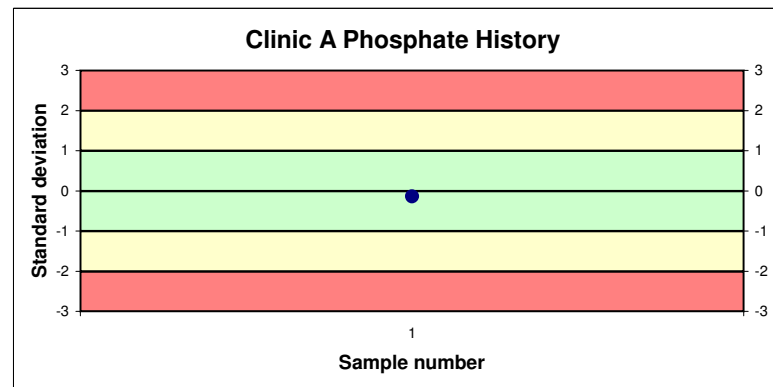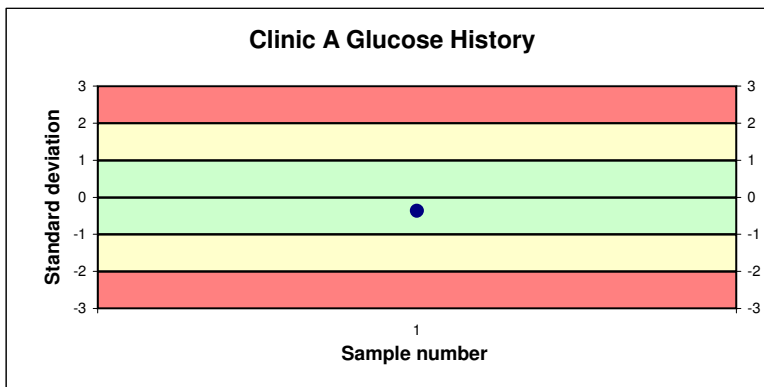

### Total Protein (g/L)

<b>Your result</b>	79	
<b>Mean of all results</b>	81	<b>Results excluded: 0</b>
- Standard deviation	5.77	
- %CV	7.12	
<b>Mean of Your analyser results</b>	81	<b>Results excluded: 0</b>
- Standard deviation	6.23	
- %CV	7.66	
<b>Your standard deviation index</b>	-0.32	
<b>NZVP result</b>	79.7	

### Urea (mmol/L)

<b>Your result</b>	18.41	
<b>Mean of all results</b>	17.17	<b>Results excluded: 0</b>
- Standard deviation	1.41	
- %CV	8.19	
<b>Mean of Your analyser results</b>	17.12	<b>Results excluded: 0</b>
- Standard deviation	1.55	
- %CV	9.07	
<b>Your standard deviation index</b>	0.83	
<b>NZVP result</b>	18.1	

